

### Continuous Radon Monitor

Model Number: 1028  
Calibration Date: 09/28/2012  
Monitor Time: 12/17/2012 23:23

Serial Number: 59237107  
CF: 2.88

### Inspector Information

Stephen R. Burns Inc.  
P.O. BOX 943  
Iowa City  
IA-52244  
Phone Number: 319-400-4844  
License Number: S00227

### Customer Information


Iowa City School System  
Van Allen Elem. Room 107  
170 Abigail AV  
North Liberty  
IA-52317

### Site & Condition

Wind:	NA	Atmospheric Condition:	NA
Year Built:	NA	Structure Type:	NA
SqFt:	NA	Monitor Location:	NA

### Test Summary

Start Time:	12/15/2012 06:14	Overall Avg:	3.0 pCi/l
End Time:	12/17/2012 06:14	EPA Avg:	3.2 pCi/l
Measurement Interval(hr):	1.0		
Elapse Time:	2 Days 0 hrs		

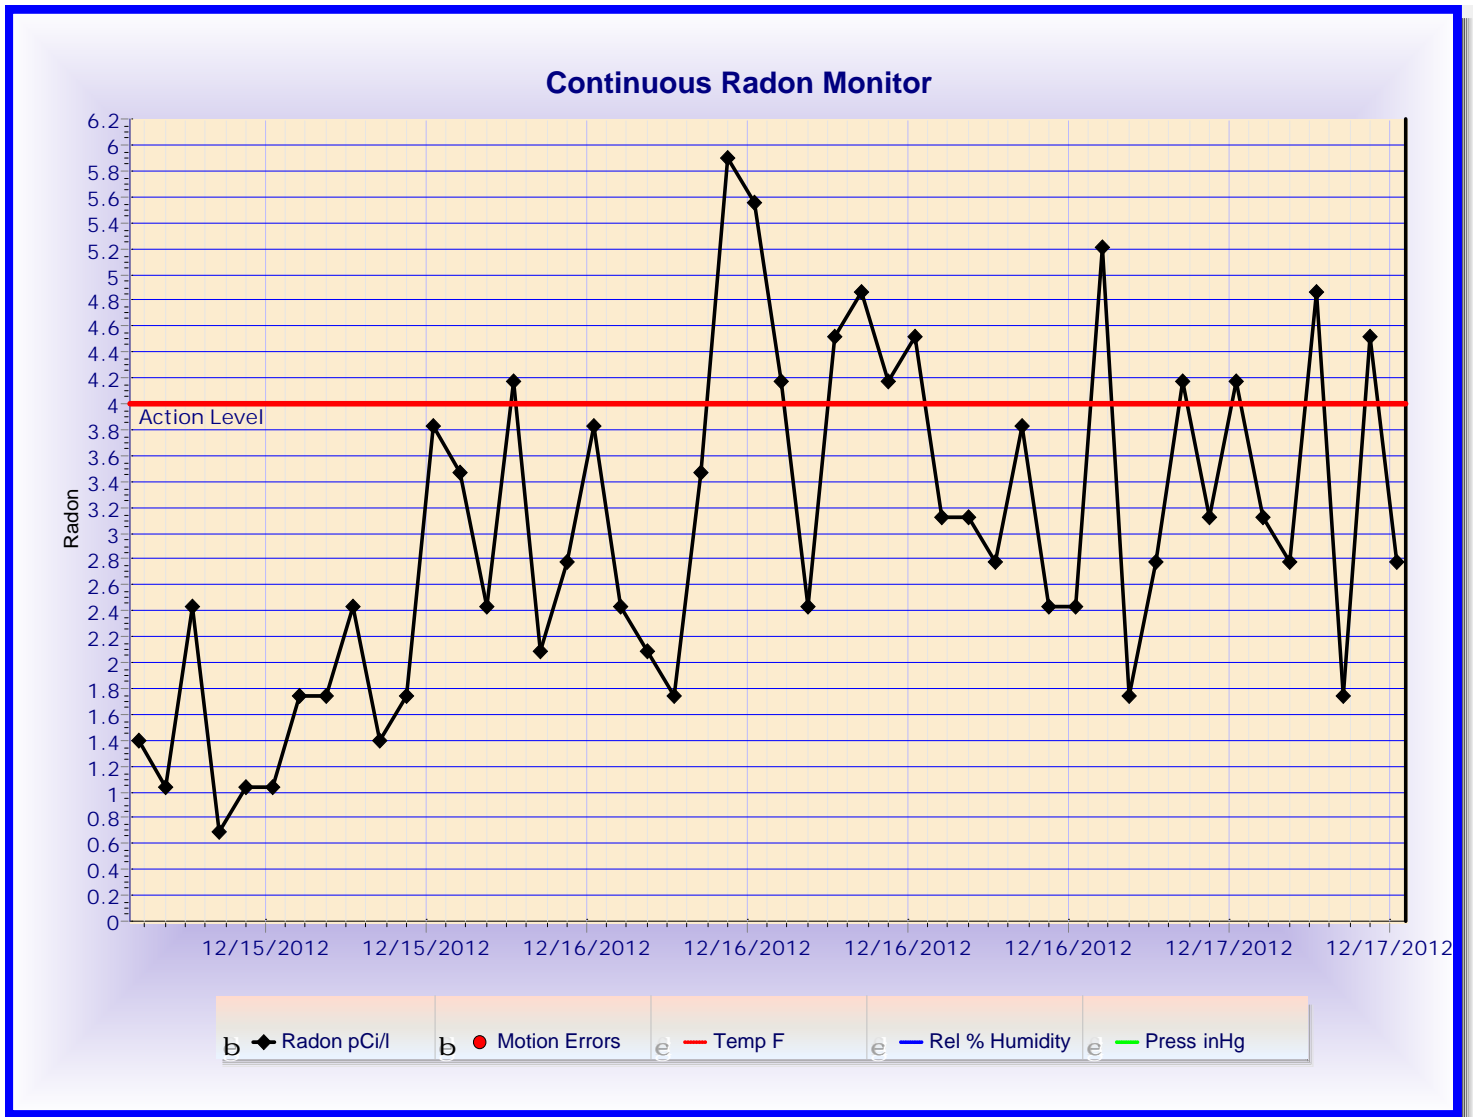

\*\*\*\*\* 12/15/2012 \*\*\*\*\*

Time	Counts pCi/l	Flags
07:14	1.4	
08:14	1.0	
09:14	2.4	
10:14	0.7	
11:14	1.0	
12:14	1.0	
13:14	1.7	
14:14	1.7	
15:14	2.4	
16:14	1.4	
17:14	1.7	
18:14	3.8	
19:14	3.5	
20:14	2.4	
21:14	4.2	
22:14	2.1	
23:14	2.8	

\*\*\*\*\* 12/16/2012 \*\*\*\*\*

Time	Counts pCi/l	Flags
00:14	3.8	
01:14	2.4	
02:14	2.1	
03:14	1.7	
04:14	3.5	
05:14	5.9	
06:14	5.6	
07:14	4.2	
08:14	2.4	
09:14	4.5	
10:14	4.9	
11:14	4.2	
12:14	4.5	
13:14	3.1	
14:14	3.1	
15:14	2.8	
16:14	3.8	
17:14	2.4	
18:14	2.4	
19:14	5.2	
20:14	1.7	
21:14	2.8	
22:14	4.2	
23:14	3.1	

\*\*\*\*\* 12/17/2012 \*\*\*\*\*

Time	Counts pCi/l	Flags
00:14	4.2	

\*\*\*\*\* 12/17/2012 \*\*\*\*\*

Time	Counts pCi/l	Flags
01:14	3.1	
02:14	2.8	
03:14	4.9	
04:14	1.7	
05:14	4.5	
06:14	2.8	

Error Flags:

M Motion:

Inspector Signature \_\_\_\_\_

PC Software Version: 2.1.1.0

Embedded Software Version: 108