

Continuous Radon Monitor

Model Number: 1028
Calibration Date: 09/28/2012
Monitor Time: 12/26/2012 10:10

Serial Number: 57077193
CF: 2.97

Inspector Information

Stephen R. Burns, Inc
P.O. Box 943
Iowa City
IA-52244
Phone Number: 319-400-4844
License Number: S00227

Customer Information


Hoover Elementary
Room 23
2200 Court ST
Iowa City
IA-52245

Site & Condition

Wind: NA
Year Built: NA
SqFt: NA
Atmospheric Condition: NA
Structure Type: NA
Monitor Location: NA

Test Summary

Start Time: 12/24/2012 09:50
End Time: 12/26/2012 09:50
Measurement Interval(hr): 1.0
Elapse Time: 2 Days 0 hrs
Overall Avg: 0.4 pCi/l
EPA Avg: 0.4 pCi/l

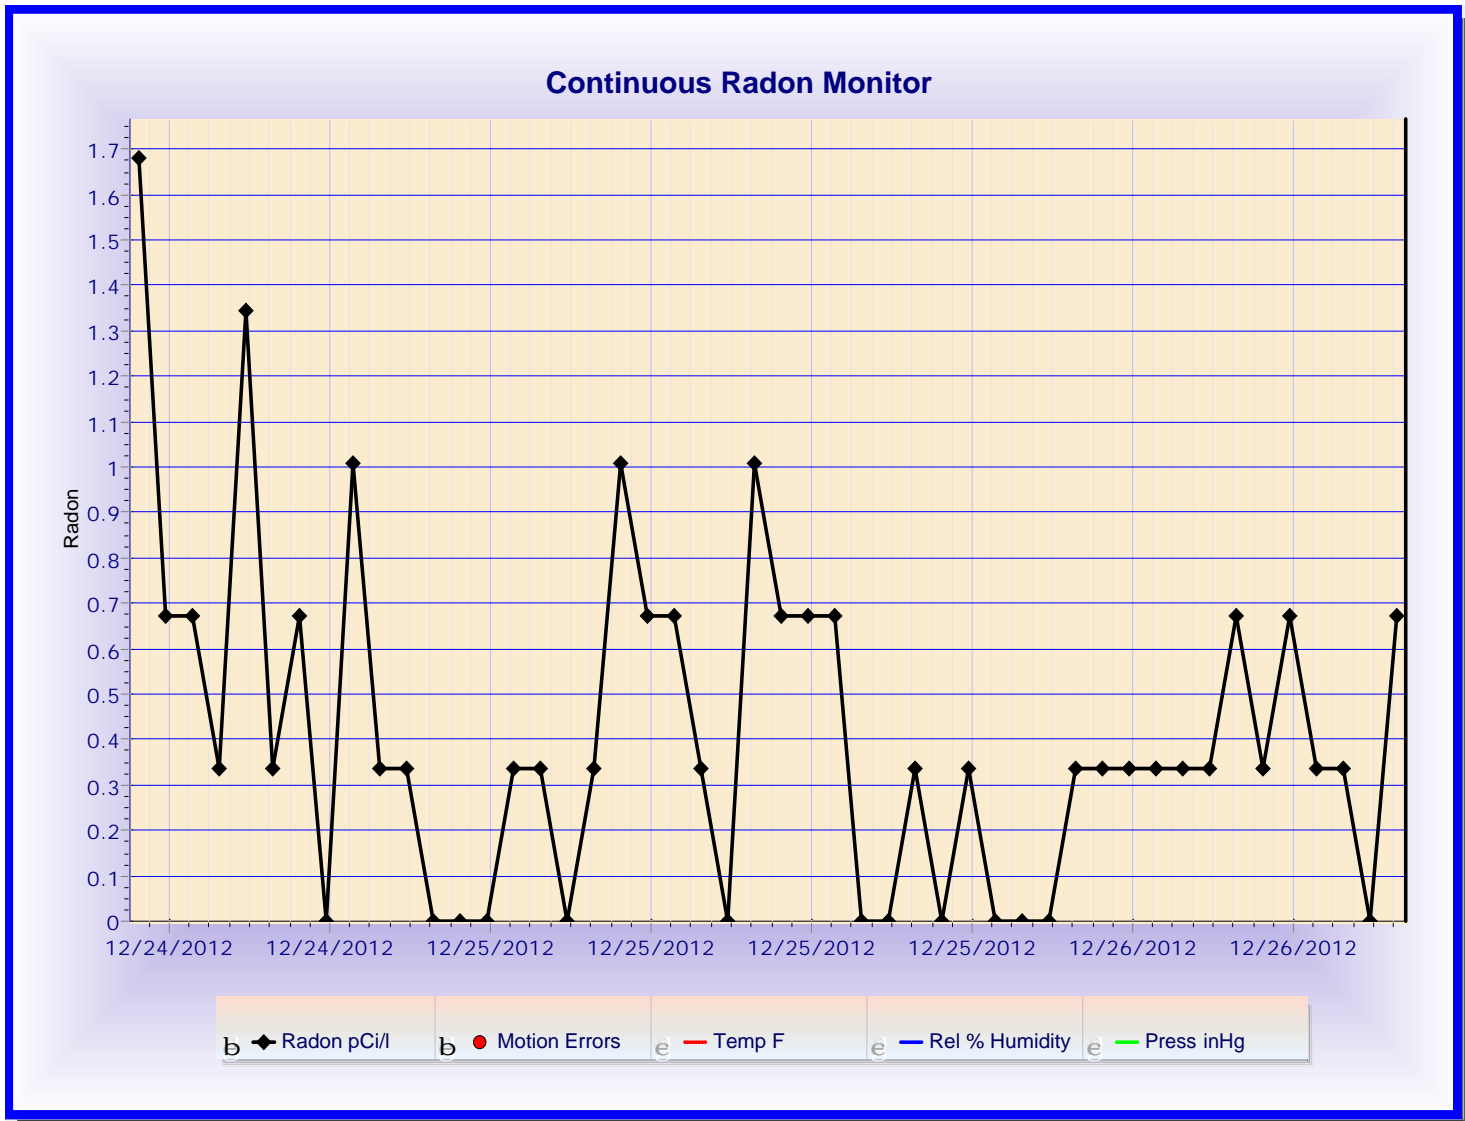

***** 12/24/2012 *****

Time	Counts pCi/l	Flags
10:50	1.7	
11:50	0.7	
12:50	0.7	
13:50	0.3	
14:50	1.3	
15:50	0.3	
16:50	0.7	
17:50	0.0	
18:50	1.0	
19:50	0.3	
20:50	0.3	
21:50	0.0	
22:50	0.0	
23:50	0.0	

***** 12/25/2012 *****

Time	Counts pCi/l	Flags
00:50	0.3	
01:50	0.3	
02:50	0.0	
03:50	0.3	
04:50	1.0	
05:50	0.7	
06:50	0.7	
07:50	0.3	
08:50	0.0	
09:50	1.0	
10:50	0.7	
11:50	0.7	
12:50	0.7	
13:50	0.0	
14:50	0.0	
15:50	0.3	
16:50	0.0	
17:50	0.3	
18:50	0.0	
19:50	0.0	
20:50	0.0	
21:50	0.3	
22:50	0.3	
23:50	0.3	

***** 12/26/2012 *****

Time	Counts pCi/l	Flags
00:50	0.3	

***** 12/26/2012 *****

Time	Counts pCi/l	Flags
01:50	0.3	
02:50	0.3	
03:50	0.7	
04:50	0.3	
05:50	0.7	
06:50	0.3	
07:50	0.3	
08:50	0.0	
09:50	0.7	

Error Flags:

M Motion:

Inspector Signature _____

PC Software Version: 2.1.1.0

Embedded Software Version: 108