

Continuous Radon Monitor

Model Number: 1028
Calibration Date: 03/16/2012
Monitor Time: 12/27/2012 15:15

Serial Number: 49745118
CF: 2.53

Inspector Information

Stephen R. Burns, Inc.
P.O. Box 943
Iowa City
IA-52244
Phone Number: 319-400-4844
License Number: S00227

Customer Information


Hills Elementary
Room 24
301 W. Main ST
Hills
IA-52235

Site & Condition

Wind:	NA	Atmospheric Condition:	NA
Year Built:	NA	Structure Type:	NA
SqFt:	NA	Monitor Location:	NA

Test Summary

Start Time:	12/24/2012 08:18	Overall Avg:	0.6 pCi/l
End Time:	12/26/2012 08:18	EPA Avg:	0.6 pCi/l
Measurement Interval(hr):	1.0		
Elapse Time:	2 Days 0 hrs		

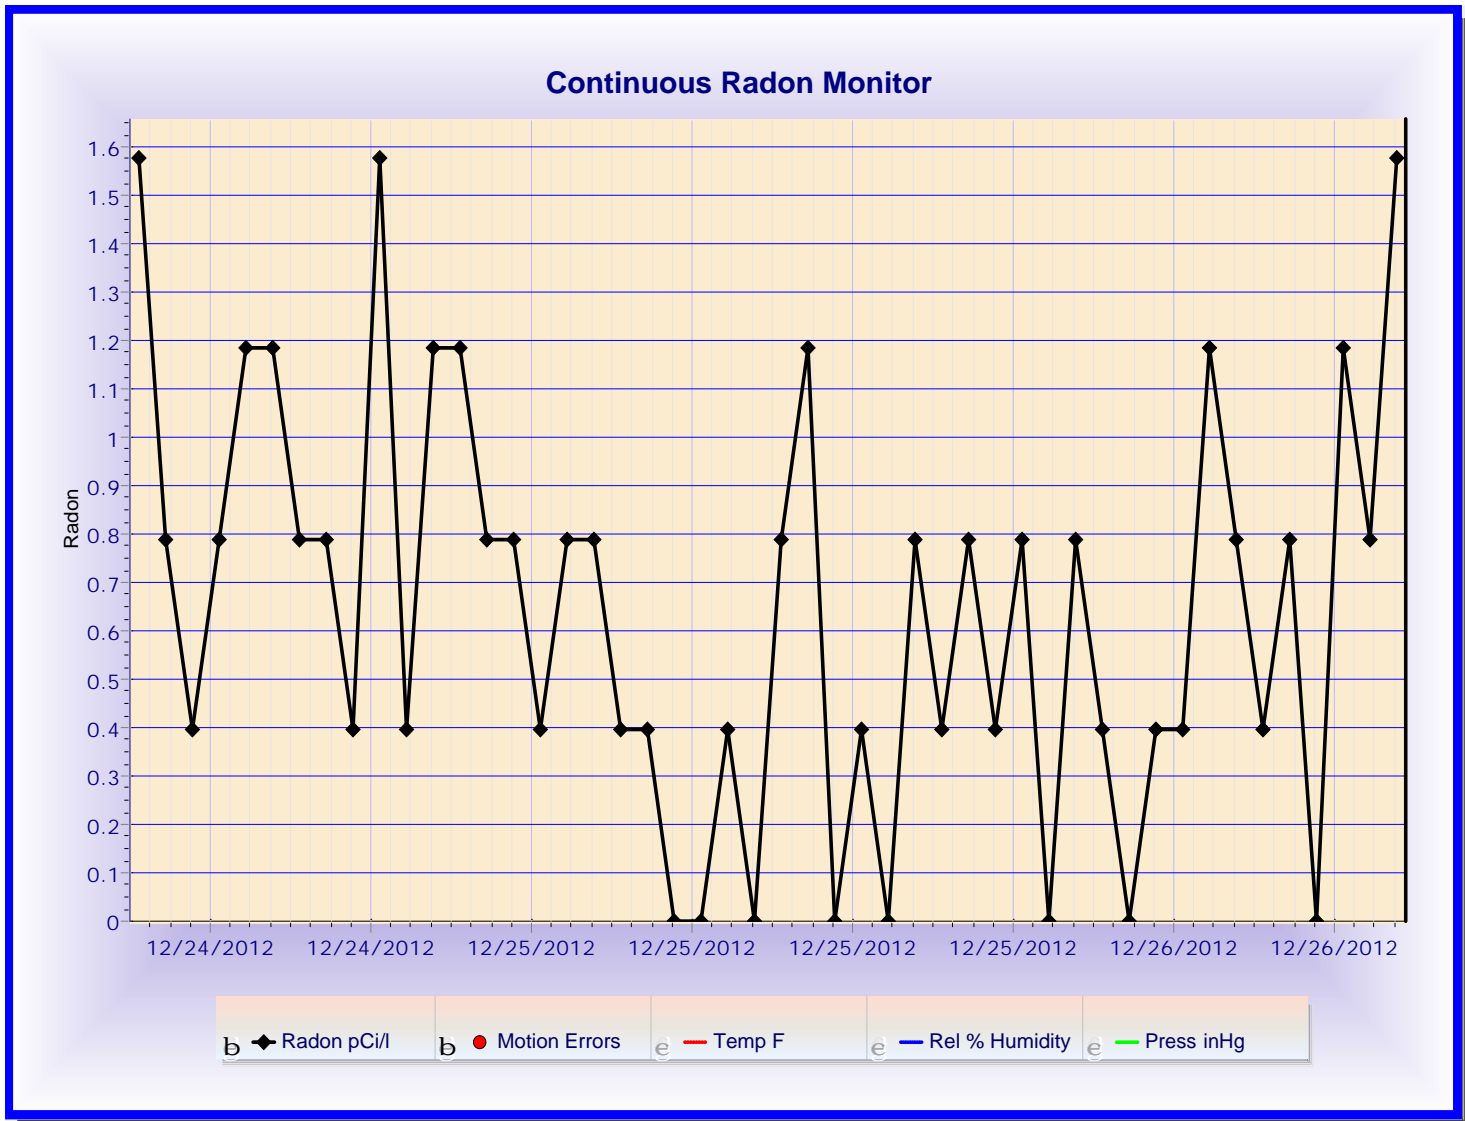

***** 12/24/2012 *****

Time	Counts pCi/l	Flags
09:18	1.6	
10:18	0.8	
11:18	0.4	
12:18	0.8	
13:18	1.2	
14:18	1.2	
15:18	0.8	
16:18	0.8	
17:18	0.4	
18:18	1.6	
19:18	0.4	
20:18	1.2	
21:18	1.2	
22:18	0.8	
23:18	0.8	

***** 12/25/2012 *****

Time	Counts pCi/l	Flags
00:18	0.4	
01:18	0.8	
02:18	0.8	
03:18	0.4	
04:18	0.4	
05:18	0.0	
06:18	0.0	
07:18	0.4	
08:18	0.0	
09:18	0.8	
10:18	1.2	
11:18	0.0	
12:18	0.4	
13:18	0.0	
14:18	0.8	
15:18	0.4	
16:18	0.8	
17:18	0.4	
18:18	0.8	
19:18	0.0	
20:18	0.8	
21:18	0.4	
22:18	0.0	
23:18	0.4	

***** 12/26/2012 *****

Time	Counts pCi/l	Flags
00:18	0.4	

***** 12/26/2012 *****

Time	Counts pCi/l	Flags
01:18	1.2	
02:18	0.8	
03:18	0.4	
04:18	0.8	
05:18	0.0	
06:18	1.2	
07:18	0.8	
08:18	1.6	

Error Flags:

M Motion:

Inspector Signature _____

PC Software Version: 2.1.1.0

Embedded Software Version: 108